

E13-2005-69

Yu. A. Batusov\*, Yu. S. Kovaliev, L. M. Soroko

CONFOCAL SCANNING MICROSCOPE FOR  
NUCLEAR PHOTOEMULSION

Submitted to «Nuclear Instruments and Methods, A, Letter to the Editor»

---

\* Corresponding author: Joint Institute for Nuclear Research, DLNP,  
141980 Dubna, Moscow Region, Joliot-Curie st., 6  
Fax: (7-09621) 66-666  
E-mail: yuabat@nusun.jinr.ru

Батусов Ю. А., Ковалев Ю. С., Сороко Л. М. E13-2005-69  
Конфокальный сканирующий микроскоп для ядерной фотоэмульсии

Описывается применение конфокального сканирующего микроскопа к объектам, находящимся в ядерной фотоэмульсии. Приведен массив из 27 микрофотограмм *одиночного* зерна серебра. Представлены поперечные сечения одного и того же следа частицы диаметром 1 мкм, которые были получены при помощи конфокального сканирующего микроскопа с открытой и с кольцевой апертурами. Показано, что конфокальный сканирующий микроскоп открывает в действительности новые возможности метода ядерной фотоэмульсии и пути получения ранее недоступной информации для физики короткоживущих частиц.

Работа выполнена в Лаборатории ядерных проблем им. В. П. Дзелепова ОИЯИ.

Препринт Объединенного института ядерных исследований. Дубна, 2005

Batusov Yu. A., Kovaliev Yu. S., Soroko L. M. E13-2005-69  
Confocal Scanning Microscope for Nuclear Photoemulsion

The application of the confocal scanning microscope to the objects in the nuclear photoemulsion is described. An array of 27 microtomograms of *single* silver grain is shown. The cross sections of the same particle track of diameter 1  $\mu\text{m}$ , detected by means of the confocal scanning microscope with open and annular apertures, are presented. It was shown that the confocal scanning microscope opens indeed new opportunities for the nuclear photoemulsion technique to get previously inaccessible information for physics of the short-living particles.

The investigation has been performed at the Dzhelepov Laboratory of Nuclear Problems, JINR.

Preprint of the Joint Institute for Nuclear Research. Dubna, 2005

New power accelerators of the particles of energy up to  $10^{11}$  eV allow one to accomplish the investigations of the interactions of the relativistic nuclei with matter by means of the laboratory facilities.

Among many experimental techniques the nuclear photoemulsion provides extremely high spatial resolution. To detect selectively straight-line particle tracks with predominant orientation in space, some new optical microscopes were constructed [1, 2].

Meanwhile, some principal problems remained nonresolved in the nuclear emulsion technique. For example, such a problem arose in the course of observation of the events with extremely many secondary particles, approximately 150. Here we observe a «shadow effect», which obscures completely the vertex of the event, and excludes the information about short-lived particles. Just from this information, we can investigate new hyperfragments with  $\Lambda$  particles inside the nucleus as well as supernuclei with  $\Lambda_c^+$  and  $\Lambda_b^+$  hyperons and fragmentation processes in the course of decay of the relativistic nuclei in flight.

The second problem is the electric charge of the secondary nuclei observed in such exotic processes. To increase the precision of this estimation, we must know the structure of the cross section of the particle track besides its width.

Finally, an interest has arisen anew to the problem of submicronic structure of *single* silver grain of the particle track. The drawback of the conventional optical microscope consists in the fact that we can see only a shadow projection of silver grains. The internal or submicronic structure is absent because of bad spatial resolution.

In this letter, we show that all these problems can be resolved by means of the confocal scanning microscope, which has never been used up to now for this aim.

A confocal scanning transmitting optical microscope, shown in Fig.1, is provided with two microobjectives, the illuminating and the imaging one, and with point-like photodetector. At every instant of time, only one microscopic part of the three-dimensional (3D) object is illuminated and detected. The 3D-image of the 3D-object is stored in the computer memory.

The performance of any microscope is described by the point spread function  $g(x, y, z)$ , so the amplitude of the image  $u(x, y, z)$  can be written as 3D-convolution  $\otimes$  of the amplitude transmittance  $t(x, y, z)$  of the 3D-object with point spread function:

$$u(x, y, z) = g(x, y, z) \otimes t(x, y, z). \quad (1)$$

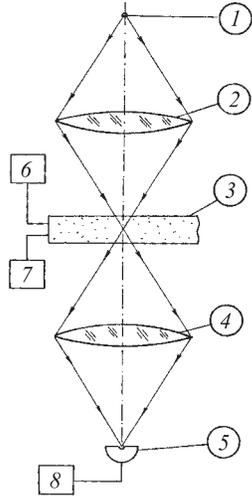


Fig. 1. Principal scheme of the confocal scanning transmitted optical microscope: 1 — point-like light source, 2 — illuminating objective, 3 — object, 4 — imaging objective, 5 — point-like detector, 6 — moving ( $x$ - $y$ ) stage, 7 — moving  $z$  stage

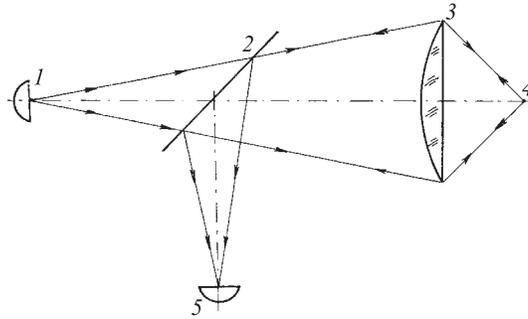


Fig. 2. Principal scheme of the reflected confocal scanning microscope: 1 — point-like light source, 2 — semitransparent mirror, 3 — objective, 4 — object, 5 — point-like detector

The amplitude point spread function of the confocal scanning transmitting microscope is equal to the product of two amplitude spread functions, that of the illuminating objective  $g_1(x, y, z)$  and that of the imaging objective  $g_2(x, y, z)$ :

$$g_2(x, y, z) = g_1(x, y, z) \cdot g_2(x, y, z). \quad (2)$$

Due to this, the lateral and axial spatial resolutions of the confocal scanning transmitting microscope will be about twice as good as in the equivalent optical microscope.



Fig. 3. General view of the SOLAR TII confocal microscope



Fig. 4. View of the particle track in the nuclear photoemulsion layer at fixed  $z$  coordinate, detected by means of the confocal scanning microscope SOLAR TII

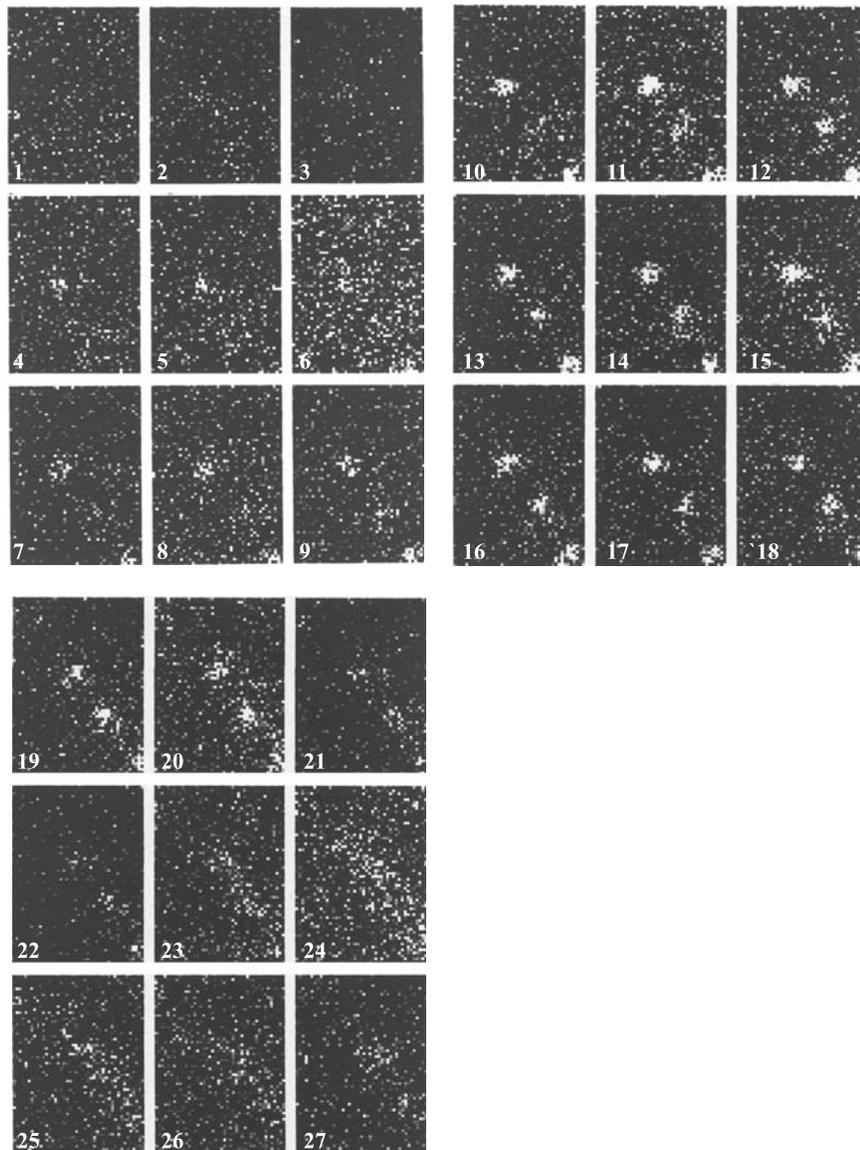


Fig. 5. Array of 27 microtomograms of *single* silver grain in the nuclear photoemulsion layer, detected at depth step  $\Delta z = 100$  nm, and at the transfer coordinate steps  $\Delta x = \Delta y = 66$  nm. The wave length  $\lambda = 0.4416 \mu\text{m}$ . Open aperture of the objective

Principal scheme of the reflected confocal scanning microscope which was used in our experiments is shown in Fig. 2. General view of this microscope, SOLAR TII, is presented in Fig. 3. The wave length  $\lambda = 0.4416 \mu\text{m}$ , the angular aperture of the objective  $\Omega = 0.9$ , the magnification is  $\times 100$ , and the field of view is equal to  $10 \times 10 \mu\text{m}$ . We also used the microobjective which was provided with annular aperture.

The view of the particle track in the nuclear photoemulsion at fixed  $z$  coordinate, detected at open aperture, is shown in Fig. 4.

The analysis of the confocal scanning microscope provided with microobjective having annular pupil was done in [3, 4, 5]. The transfer resolution and the depth resolution are about twice as high as in the confocal scanning microscope with open pupil. If the angular aperture of the microobjective is equal to  $90^\circ$ , then the optical resolutions  $\Delta x_2^{\text{opt}}$ , and  $\Delta z_2^{\text{opt}}$  will be equal to

$$\Delta x_2^{\text{opt}} = \Delta z_2^{\text{opt}} = \frac{\lambda}{4}. \quad (3)$$

So, for  $\lambda = 0.4 \mu\text{m}$ ,  $\Delta x_2^{\text{opt}} = \Delta z_2^{\text{opt}} = 0.1 \mu\text{m}$ .

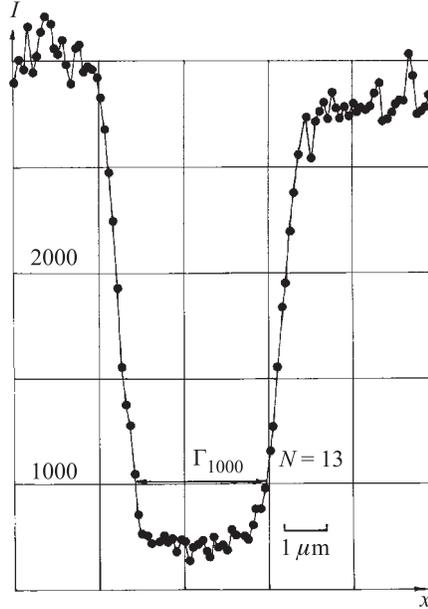


Fig. 6. The transfer intensity plot of the cross section of the particle track with width of the order of  $4 \mu\text{m}$  in the reflectory mode of scanning

By means of the confocal scanning microscope SOLAR TII with open aperture we have detected an array of 27 microtomograms of *single* silver grain in

the nuclear photoemulsion (Fig. 5). The depth step  $\Delta z$  was equal to 100 nm, and the transfer scanning steps  $\Delta x$  and  $\Delta y$  were equal to 66 nm.

The transfer intensity plot of the particle track with width of the order of  $4 \mu\text{m}$  is shown in Fig. 6.

The cross sections of the particle track with diameter of the order of  $1 \mu\text{m}$ , which were detected by means of the confocal scanning microscope with open (a) and annular (b) apertures, are shown in Fig. 7. The optical scheme of the experiment *b* is presented in Fig. 8.

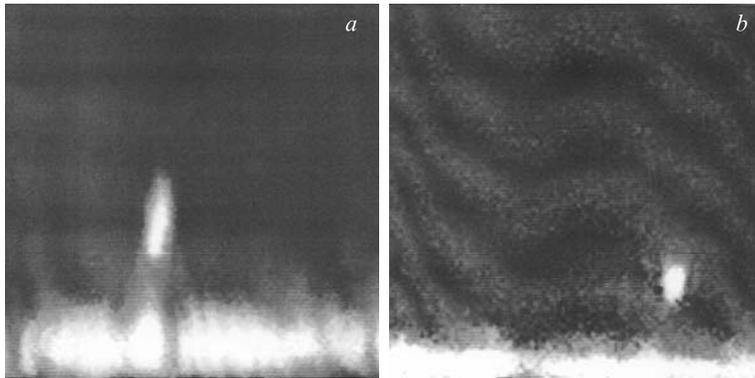


Fig. 7. Two cross sections of the particle track, obtained at different apertures: *a*) open aperture, *b*) annular aperture

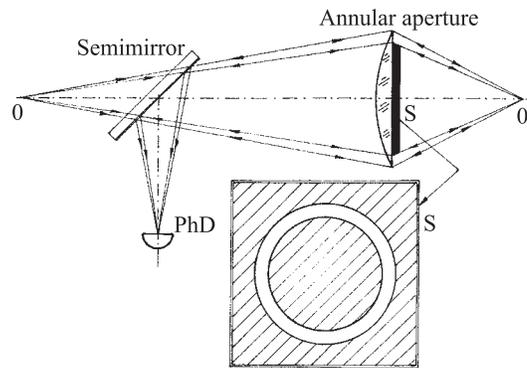


Fig. 8. The optical scheme of the confocal scanning microscope with annular aperture

**Summary.** We have shown experimentally that the confocal scanning microscope opens indeed new opportunities of the nuclear photoemulsion technique

to get previously inaccessible information. It provides submicronic spatial resolution. It suppresses the «shadow effect» in the vertex region of the event with a very high number ( $\sim 150$ ) of the secondary particles. It gives supermicronic estimation of the internal structure of *single* silver grain.

**Acknowledgements.** The authors wish to thank Prof. V.L. Aksenov and S. I. Tyutyunnikov for support and useful discussions.

## REFERENCES

1. *Astakhov A. Yu. et al.* Meso-optical Fourier transform microscope — a new device for high energy physics. // Nucl. Instr. Meth. A. 1989. V. 283. P. 13–23.
2. *Astakhov A. Yu. et al.* Dark-field scanning confocal microscope for vertical particle track in nuclear emulsion. JINR Commun. E13-99-342. Dubna, 1999.
3. *Wilson T., Sheppard C.* Theory and practice of scanning optical microscopy. London: Academic Press, 1984.
4. *Sheppard C. J. R., Wilson T.* Image formation in confocal optical systems. SPIE 232, Book II. 1980. P. 197–202.
5. *Gu M., Sheppard C. J.* Three-dimensional imaging in confocal fluorescent microscopy with annular lenses. // J. Mod. Opt. 1991. V. 38. P. 2247–2263.

Received on May 24, 2005.

Редактор *Н. С. Скокова*

Подписано в печать 28.07.2005.

Формат 60 × 90/16. Бумага офсетная. Печать офсетная.

Усл. печ. л. 0,68. Уч.-изд. л. 0,96. Тираж 305 экз. Заказ № 54978.

Издательский отдел Объединенного института ядерных исследований  
141980, г. Дубна, Московская обл., ул. Жолио-Кюри, 6.

E-mail: [publish@pds.jinr.ru](mailto:publish@pds.jinr.ru)

[www.jinr.ru/publish/](http://www.jinr.ru/publish/)